



UNIVERSITY OF
BIRMINGHAM



Towards efficient neutron spectroscopy with a Nitrogen-filled Spherical Proportional Counter


I. Manthos¹, I. Giomataris², I. Katsioulas¹, P. Knights¹, T. Neep¹, K. Nikolopoulos¹, T. Papaevangelou², B. Phoenix¹ and R. Ward¹

¹ University of Birmingham, School of Physics and Astronomy, Birmingham, United Kingdom

² CEA-Saclay, IRFU, Gif-sur-Yvette, France

HEPP & APP Annual Conference 2022

5/4/2022 RAL-STFC, Oxfordshire, UK

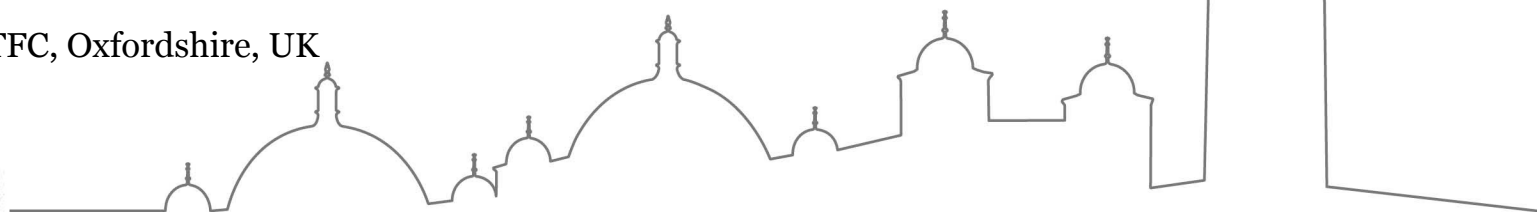

This research has been funded by the European Union's Horizon 2020 Research and Innovation Programme under the Marie Skłodowska-Curie Grant Agreement No 845168 (neutronSphere)

Neutron spectroscopy with the Spherical Proportional Counter




UNIVERSITY OF
BIRMINGHAM

Dark matter underground experiments

- MeV neutrons produce signals in the region of interest for WIMP detection
 - Sources: Radioactivity of cavern, muon induced hadronic and electromagnetic showers (cosmic rays)
 - Elastic scattering with target nuclei of gas, interaction with detector material
- Neutron background can not be discriminated using event properties
- Neutron rejection: shielding and use of high-purity materials.
- Data analysis require an estimation of the neutron background expected in order to compare with the observed number of events.

Current neutron detector status

^3He proportional counters



Efficient for thermal and fast neutrons, low efficiency in γ -rays



Wall effect \rightarrow high pressure (impractical)
 ^3He extremely expensive



The Spherical Proportional Counter

Electric field scales as $1/r^2$

- Divided into “drift” and “amplification” regions

$$\vec{E} = \frac{V_1}{r^2} \frac{r_c r_a}{r_c - r_a} \hat{r} \approx \frac{V_1}{r^2} r_a$$

Capacitance independent of detector size



- Low electronic noise

r_c = cathode radius

r_a = anode radius


$$C = 4\pi\epsilon_0 \frac{r_c r_a}{r_c - r_a} \approx 4\pi\epsilon_0 r_a \sim 1\text{pF}$$

- Large gain - Single e^- threshold
- Maximum volume-to-surface ratio
- High pressure operation
- Simple, robust design with a flexibility in target gas
- Applications in n-spectroscopy to DM!

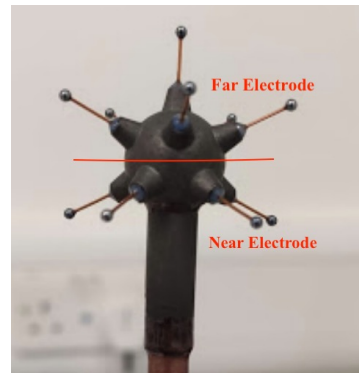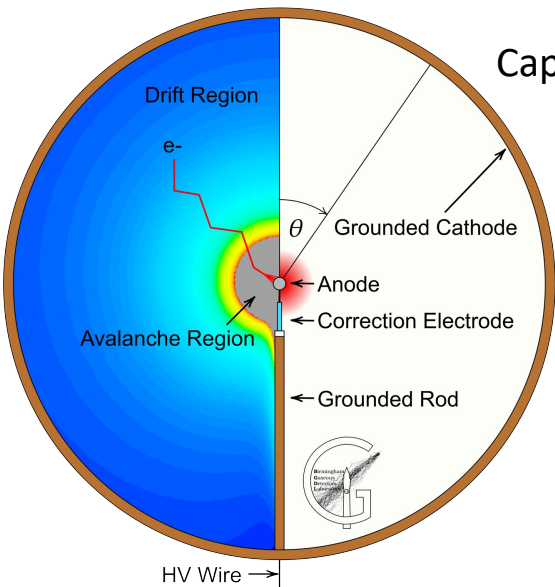

Multi anode ACHINOS sensor

- Decouples drift and amplification fields
- Allows for increased target mass

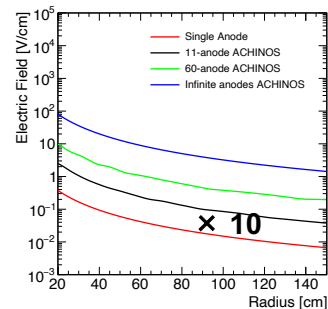



UNIVERSITY OF
BIRMINGHAM

[*I.Giomataris et al, JINST, 2008, P09007*](#)

[*I.Katsioulas et al, JINST, 13, 2018, no.11, P11006*](#)

See also next talk by I. Katsioulas
and tomorrow 11:15 by P. Knights


Neutron detection with the Spherical Proportional Counter

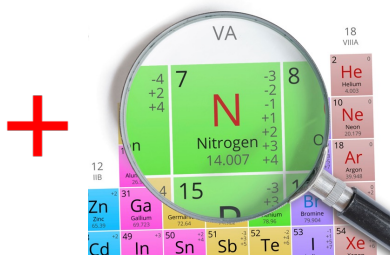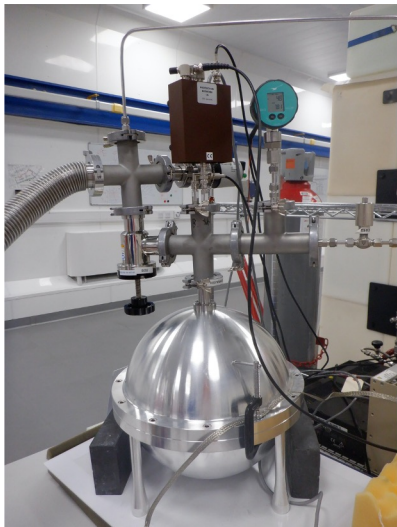


- ✓ Non-toxic
- ✓ Non-flammable
- ✓ Simple and robust setup
- ✓ Easy deployment and operation
- ✓ Cost efficient

- ✓ Wall effect suppressed due to higher atomic number of N_2 relative to 3He → lower pressure
- ✓ Good efficiency in detecting thermal neutrons in large volumes
- ✓ Low γ -ray efficiency
- ✓ Spectroscopic measurement of neutrons


Bougamont, E et al (2017). NIM A, 847, 10–14

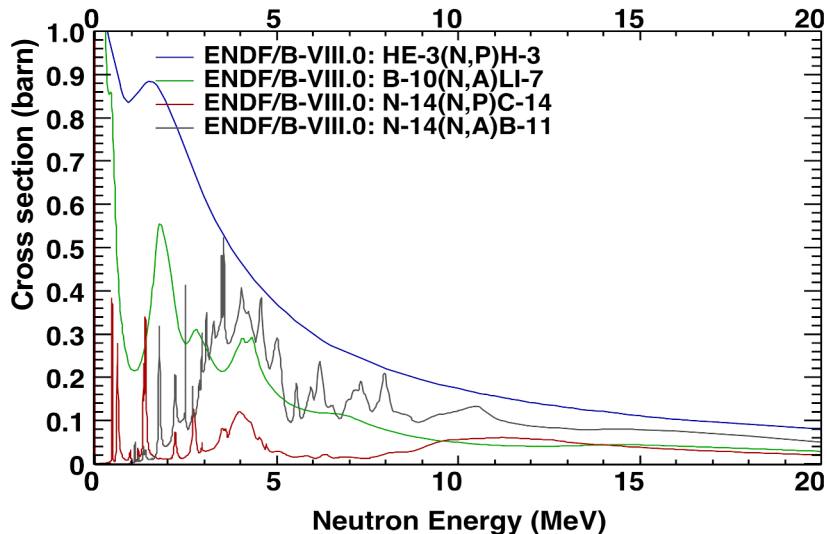

Nitrogen as target



The Graphite stack @ University of Birmingham

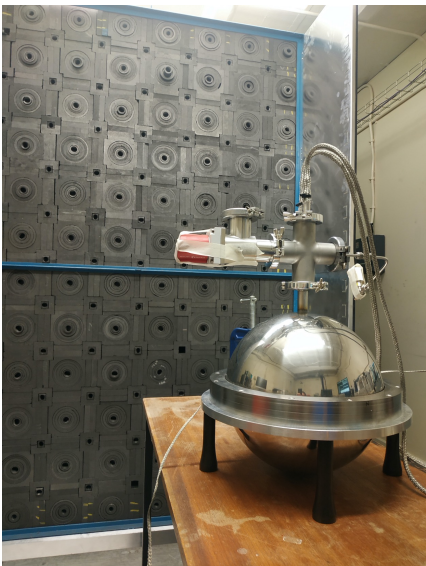


Investigate the capability of the SPC to detect fast neutrons and neutrons thermalized by the graphite.

Spherical Proportional Counter


- 30 cm Ø
- N₂ gas filling

Multi-anode sensor

- 11 anodes
- 1mm Ø
- Reading in 2 channels (near – far)

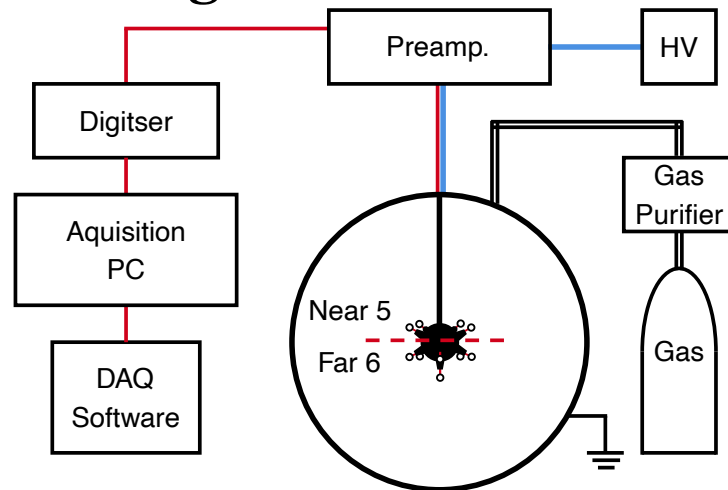

- Calibration measurements
- Thermal and fast neutrons at 1 bar and [3.6, 4.2] kV bias
- Thermal and fast neutrons at 1.5 bar and 4.5 kV bias
- Thermal neutrons at 1.8 bar and 6 kV bias

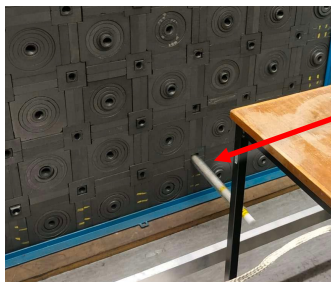




²⁴¹Am⁹Be neutron source
A = 2.6 x 10⁶ Bq

Neutron measurements with the Spherical Proportional Counter

$^{241}\text{Am}^9\text{Be}$ neutron source

1 bar N_2 , 3.6 kV

Response of near channel to thermal neutrons

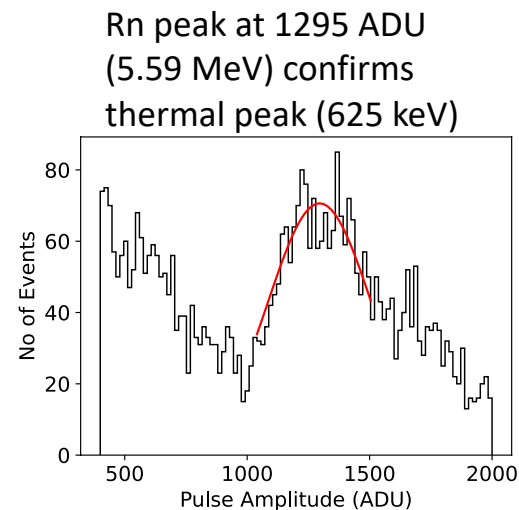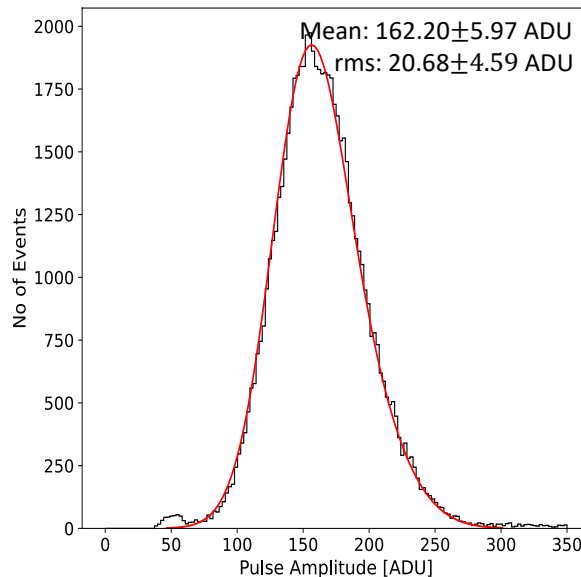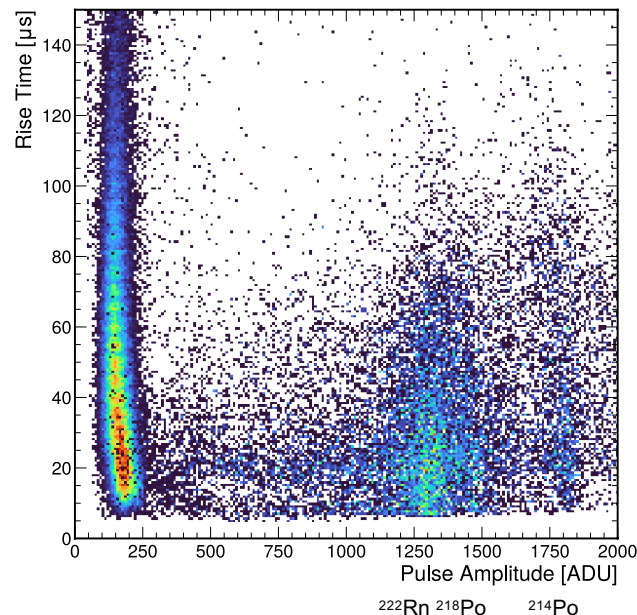


Thermal peak correspond to 625 keV recoil energy ($^{14}\text{N} + n \rightarrow ^{14}\text{C} + p + 625 \text{ keV}$)

Neutron measurements with the Spherical Proportional Counter



$^{241}\text{Am}^9\text{Be}$ neutron source

1.5 bar N_2 , 4.5 kV

- Detection of thermal and fast neutrons

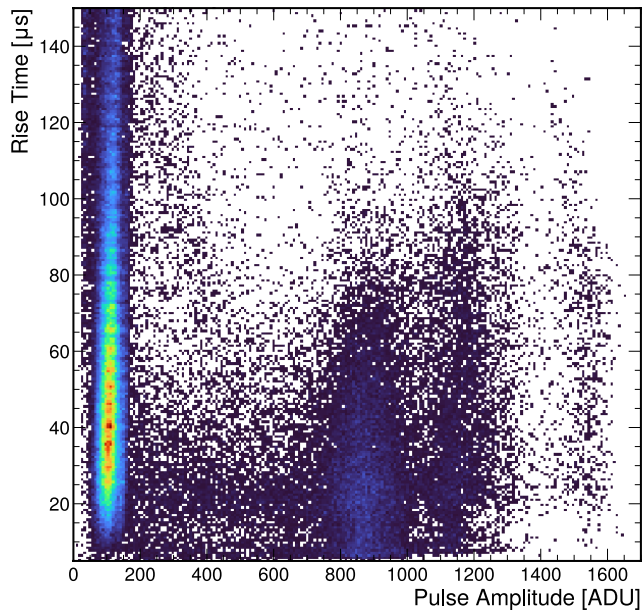

Confirmation of thermal neutrons
peak from ^{222}Rn decay peaks

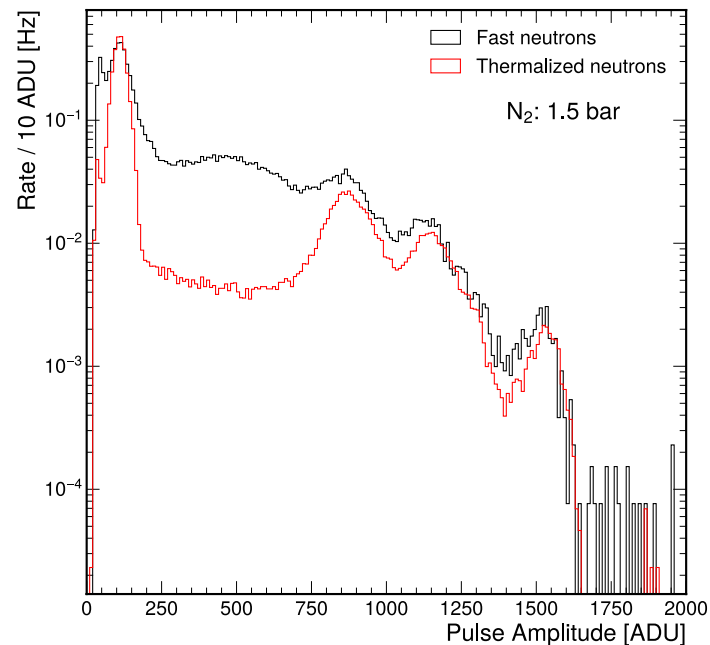
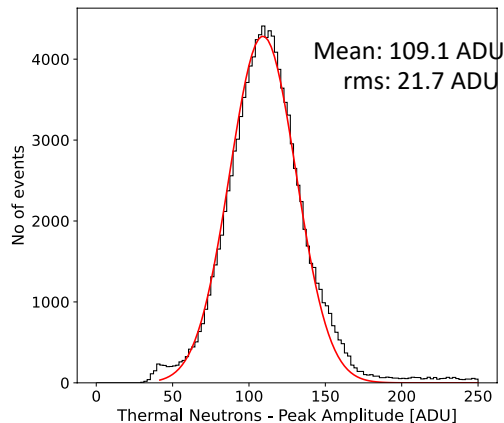


Neutron measurements with the Spherical Proportional Counter

$^{241}\text{Am}^9\text{Be}$ neutron source

1.8 bar N_2 , 6 kV

Thermal neutrons detection

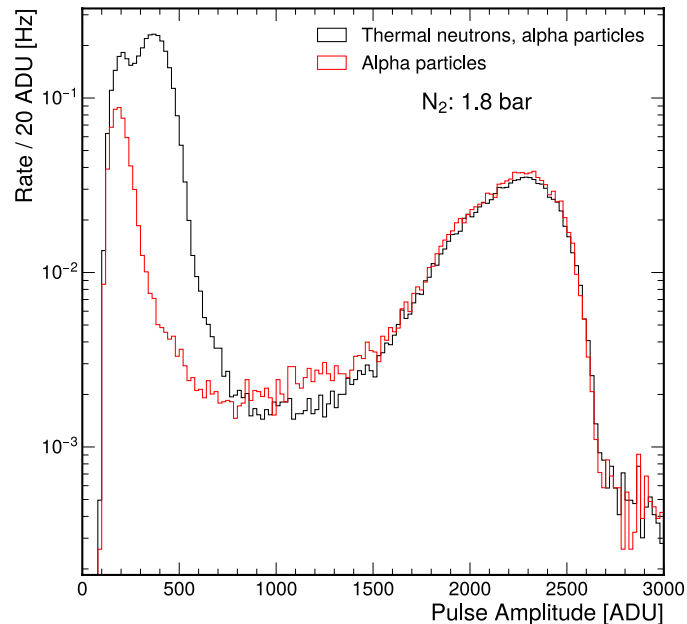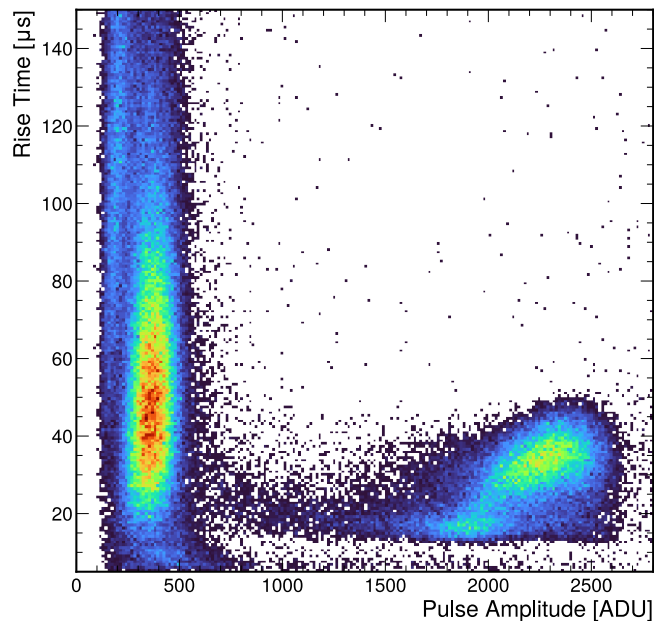

^{210}Po alpha (5.4MeV) sample, inside the detector → energy reference

Simulation of the detector response

UoB simulation framework for complete simulation of a detection setup



- GEANT4 for particle transport in a geometry and their interaction with materials
- FEM simulation (ANSYS, COMSOL) of electromagnetic fields
- Garfield++ for the generation, drift and multiplication of primary electrons and signal generation



- ✓ Differentiate protons from alphas
- ✓ Provide initial interaction point
- ✓ Identify possible wall effect

- Source activity: 2.6 MBq
 - Probability to reach detector volume $\sim 5 \times 10^{-3}$
 - Detection rate: ~ 5 Hz
- Efficiency: $\sim 3.7 \times 10^{-4}$

Simulation results \Rightarrow Efficiency: $\sim 1.9 \times 10^{-4}$

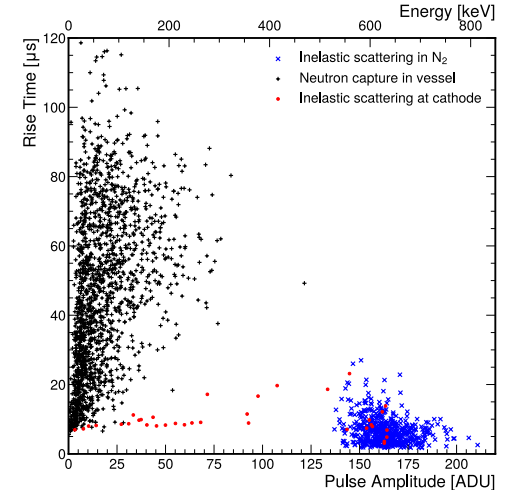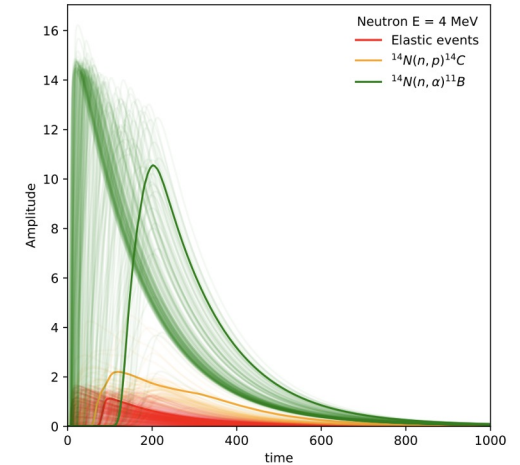

Neutron measurements at MC40 cyclotron

Spectroscopic measurement of neutron-induced dose to patients during proton therapy treatment





^9Be target on deuterium beamline

- 5.90 ± 0.08 MeV deuterons
- $^9\text{Be}(d,n)$ reaction
- Same detector setup
- Moderators used to study neutron detection (paraffin, boron doped polyethylene, lead)

Neutron measurements at MC40 cyclotron

Preliminary analysis results

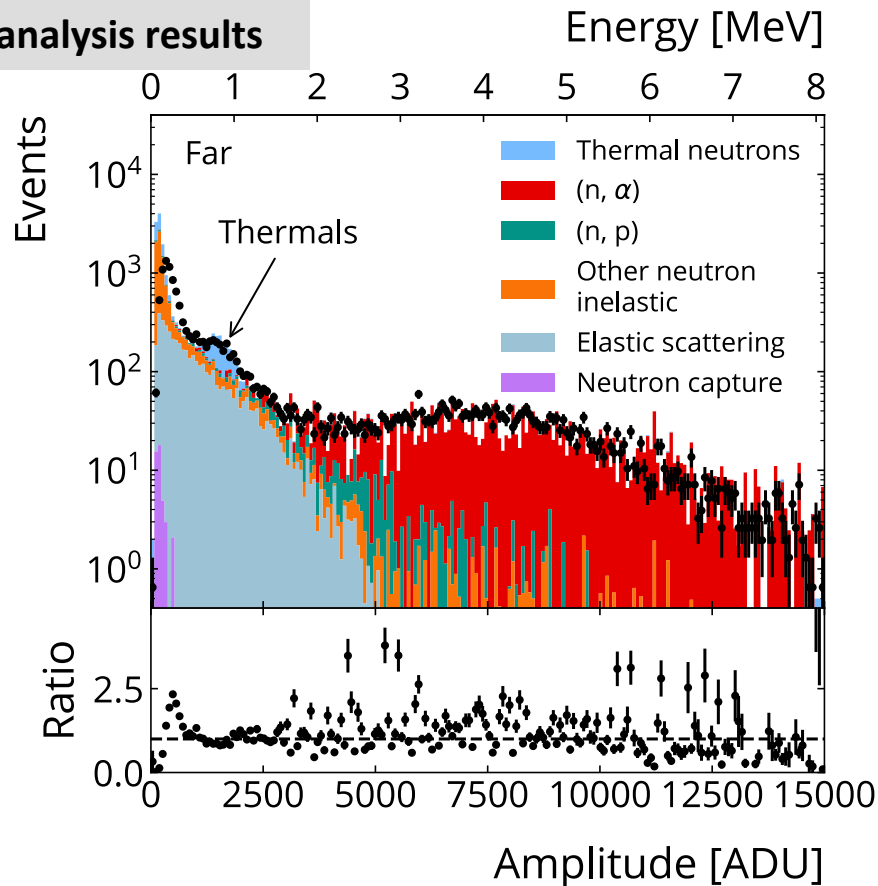
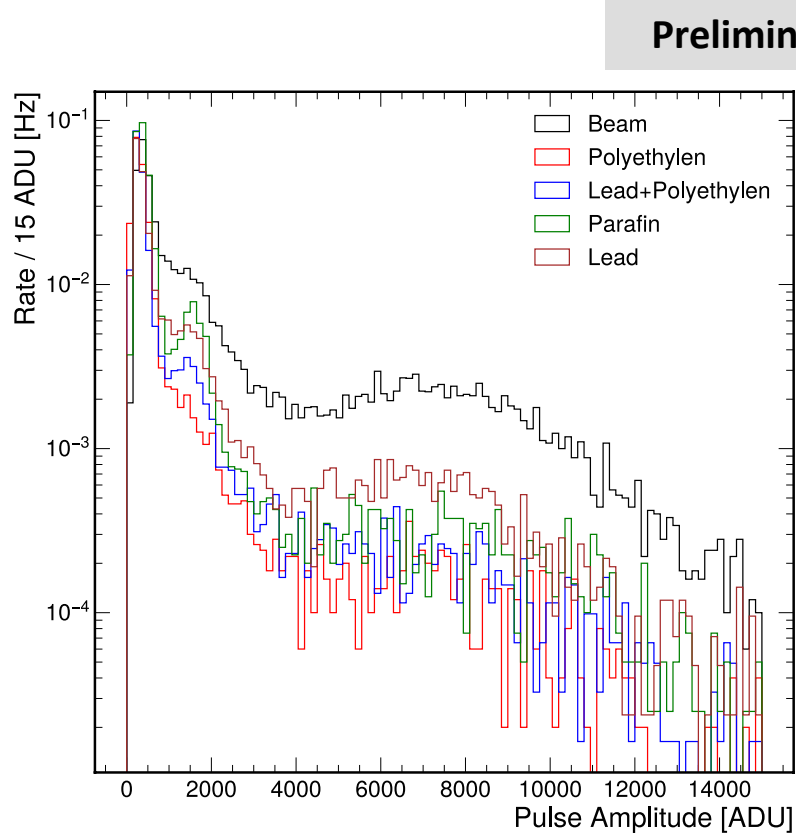


Neutron measurements at the Boulby Underground Laboratory

- Underground facility 1100 m under surface, North Yorkshire (UK)
- Instrumentation R&D and neutron measurements at controlled environment.
- 30cm Ø Spherical Proportional Counter installed and operating
- ^{252}Cf neutron source available
- Measurements in the (very) near future!





Boulby Underground Laboratory

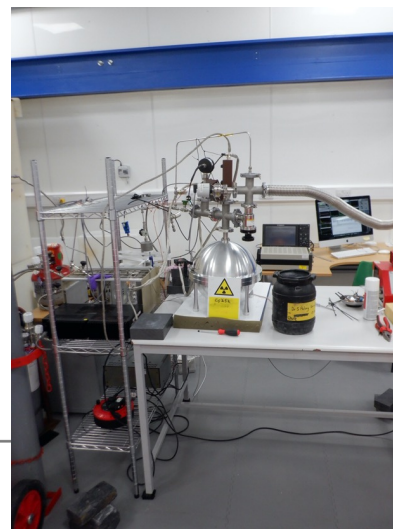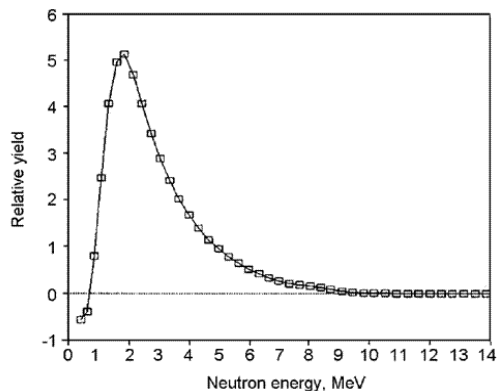

Neutron detection with the Spherical Proportional Counter

Summary

- Neutron measurements set up accomplished
- Neutron detection performed in the Graphite stack facility in Birmingham
- Medical application - Measurement of energy spectra of the neutron-induced dose to patients during proton therapy treatment sessions @ MC40 cyclotron facility (UoB)
- Corresponding measurements in Boulby
- Mono-energetic neutron measurement (@ Demokritos, Greece)

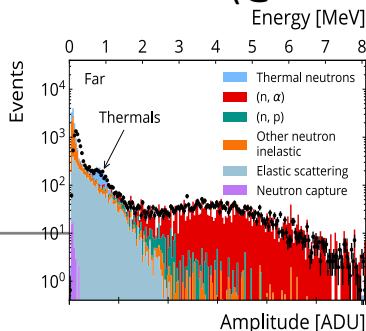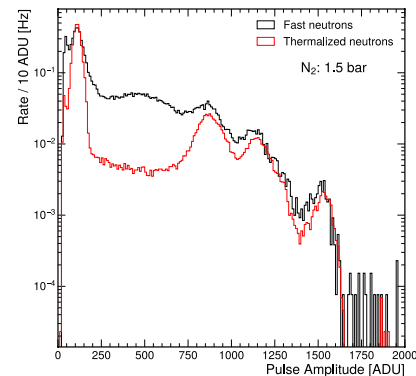

UNIVERSITY OF
BIRMINGHAM

